

Patient ID: Microchip 023 354 323
Patient name: Buetow Branson, 6. Blue
Eye Punch Female
Date of birth: 9/12/2008
Gender: Female
Gestational age: n/a
Keywords: Australian Cattle Dog

Clinic ref:
Site: Canine Companions
Veterinary Hospital
Examiner: Joanna Jones, DVM
Exam date: 10/27/2008 3:21 PM
Age on exam date: 1 month

Patient Notes

AEP, 10/27/2008 3:27 PM

bilateral hearing
no sedation

Chart 1 -- Waveforms

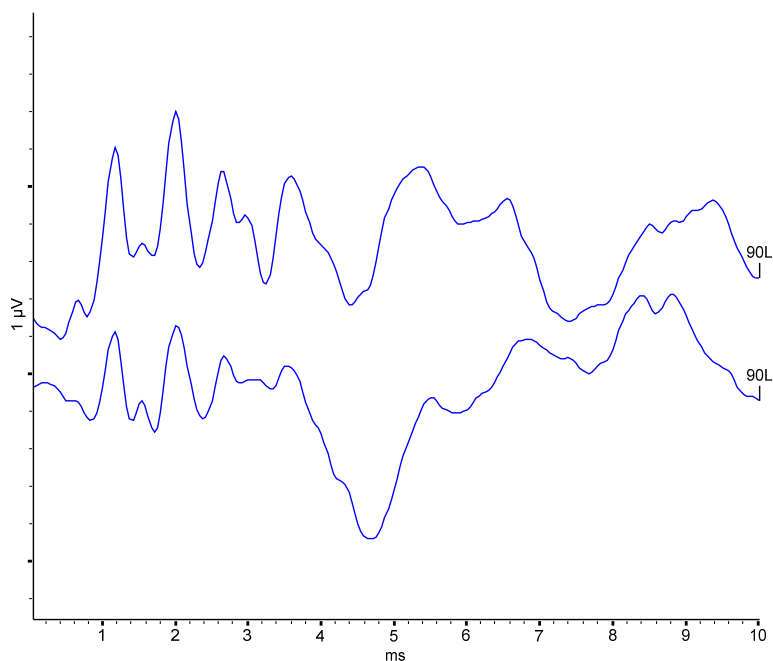


Chart 1 -- Measurements

This measurement table has not been printed because it is blank.

Chart 1 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T2 90.0 dB nHL L 33.10 Hz [1]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T1 90.0 dB nHL L 33.10 Hz [2]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T2 90.0 dB nHL L 33.10 Hz [1]	510	30.33 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Chart 1 -- Waveform details

T1 90.0 dB nHL L 33.10 Hz [2]	510	21.30 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	---------	-----------------------------	-----------------------------

Trace	Test set
T2 90.0 dB nHL L 33.10 Hz [1]	Dr. Jones Protocol
T1 90.0 dB nHL L 33.10 Hz [2]	Dr. Jones Protocol

Chart 2 -- Waveforms

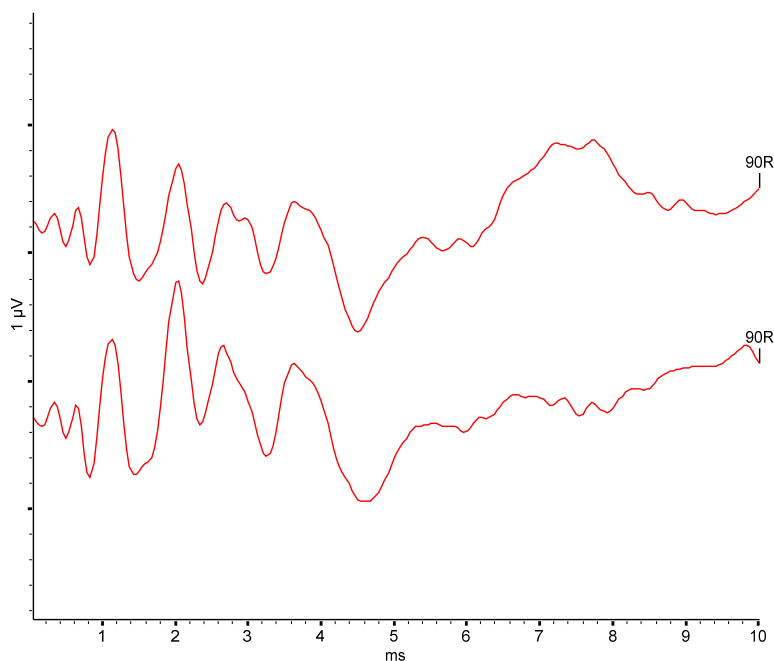


Chart 2 -- Measurements

This measurement table has not been printed because it is blank.

Chart 2 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL R 33.10 Hz [4]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T4 90.0 dB nHL R 33.10 Hz [5]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL R 33.10 Hz [4]	510	12.97 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T4 90.0 dB nHL R 33.10 Hz [5]	510	8.77 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T3 90.0 dB nHL R 33.10 Hz [4]	Dr. Jones Protocol

Chart 2 -- Waveform details

T4 90.0 dB nHL R 33.10 Hz [5]	Dr. Jones Protocol
-------------------------------	--------------------