

Patient ID: DN07542404/MC445F636933
 Patient name: Buetow Branson, Ruselrun Jet Bleu Streak
 Date of birth: 6/4/2004
 Gender: Male
 Gestational age: n/a
 Keywords: Australian Cattle Dog

Clinic ref:
 Site: Canine Companions Veterinary Hospital
 Examiner: Joanna Jones, DVM
 Exam date: 4/10/2009 4:28 PM
 Age on exam date: 4 years 10 months

Patient Notes

AEP, 4/10/2009 4:47 PM
 bilateral hearing

Chart 1 -- Waveforms

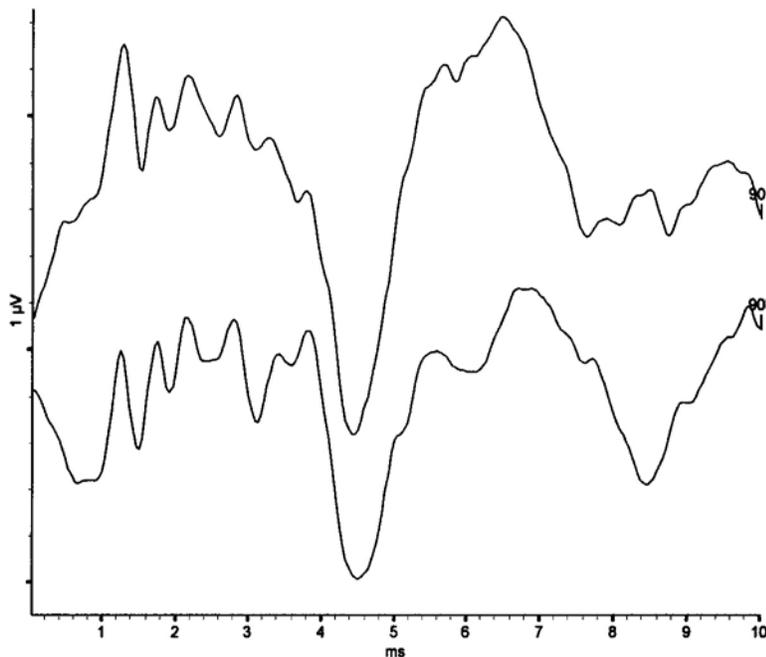


Chart 1 -- Measurements

This measurement table has not been printed because it is blank.

Chart 1 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T4 90.0 dB nHL L 33.10 Hz [4]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T3 90.0 dB nHL L 33.10 Hz [3]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T4 90.0 dB nHL L 33.10 Hz [4]	510	46.60 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct
T3 90.0 dB nHL L 33.10 Hz [3]	510	3.95 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

Chart 1 -- Waveform details

Trace	Test set
T4 90.0 dB nHL L 33.10 Hz [4]	Dr. Jones Protocol
T3 90.0 dB nHL L 33.10 Hz [3]	Dr. Jones Protocol

Chart 2 -- Waveforms

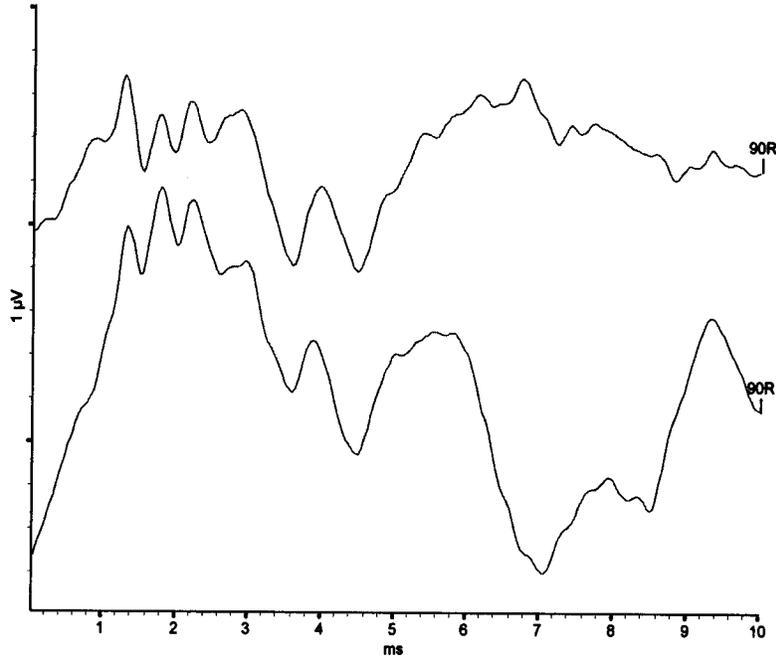


Chart 2 -- Measurements

This measurement table has not been printed because it is blank.

Chart 2 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T11 90.0 dB nHL R 33.10 Hz [10]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T8 90.0 dB nHL R 33.10 Hz [8]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T11 90.0 dB nHL R 33.10 Hz [10]	510	9.73 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct
T8 90.0 dB nHL R 33.10 Hz [8]	510	53.68 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

Trace	Test set
T11 90.0 dB nHL R 33.10 Hz [10]	Dr. Jones Protocol
T8 90.0 dB nHL R 33.10 Hz [8]	Dr. Jones Protocol