


Patient ID: DN29578101  
 Patient name: Buetow Branson, Purple Female  
 Date of birth: 11/28/2010  
 Gender: Female  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC035025546  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:05 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:13 PM**  
 bilateral hearing  
 no sedation

**Chart 1 -- Waveforms**

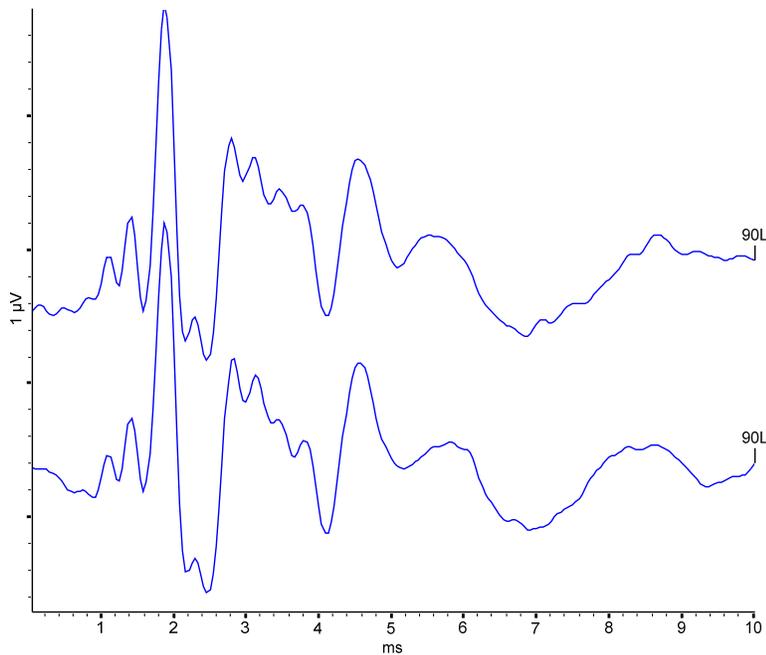

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL L 33.10 Hz [3]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T2 90.0 dB nHL L 33.10 Hz [2]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL L 33.10 Hz [3]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 1 -- Waveform details**

T2 90.0 dB nHL L 33.10 Hz [2]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T3 90.0 dB nHL L 33.10 Hz [3]	Dr. Jones Protocol
T2 90.0 dB nHL L 33.10 Hz [2]	Dr. Jones Protocol

**Chart 2 -- Waveforms**

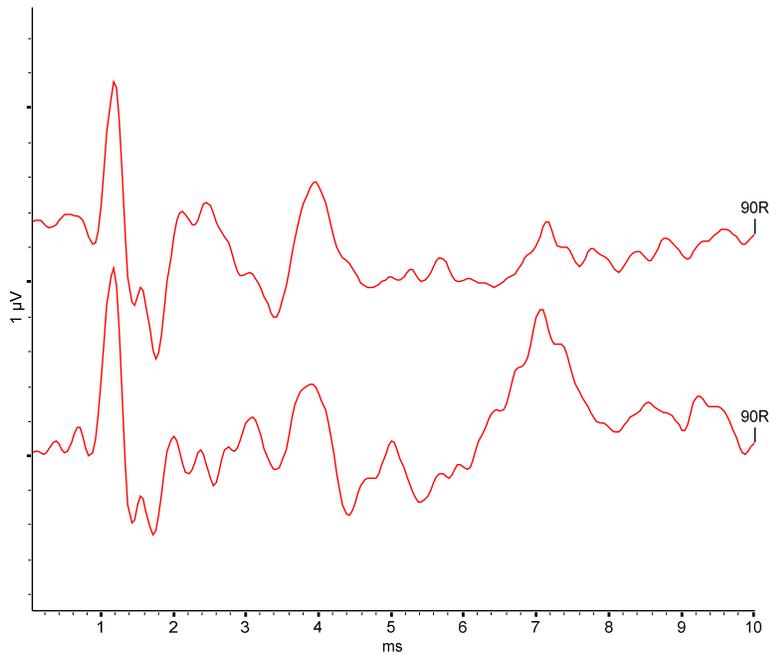

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T5 90.0 dB nHL R 33.10 Hz [6]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T6 90.0 dB nHL R 33.10 Hz [5]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T5 90.0 dB nHL R 33.10 Hz [6]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T6 90.0 dB nHL R 33.10 Hz [5]	510	1.92 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T5 90.0 dB nHL R 33.10 Hz [6]	Dr. Jones Protocol


Patient ID: DN29578102  
 Patient name: Buetow Branson, Blue Male  
 Date of birth: 11/28/2010  
 Gender: Male  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC035026809  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:16 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:23 PM**  
 Unilateral deaf - right ear  
 no sedation.

**Chart 2 -- Waveforms**

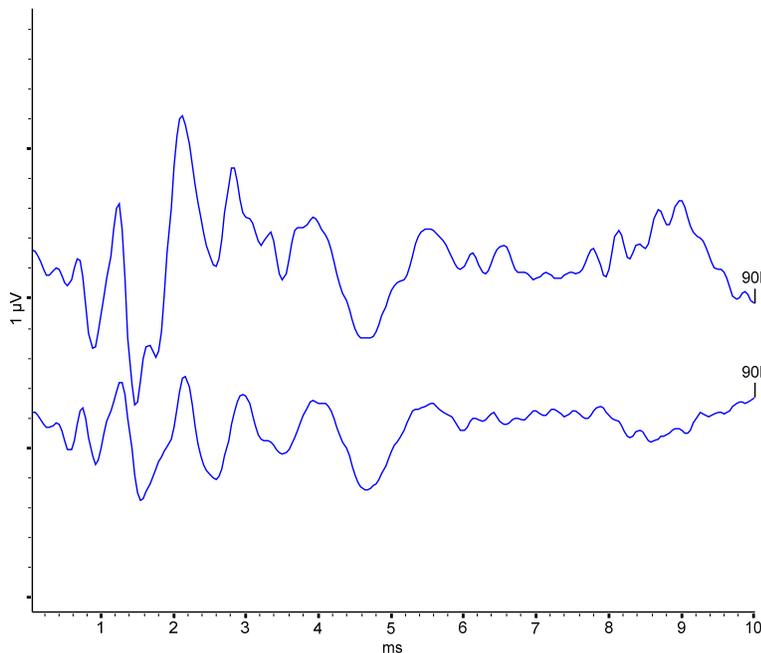

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T5 90.0 dB nHL L 33.10 Hz [7]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T3 90.0 dB nHL L 33.10 Hz [9]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T5 90.0 dB nHL L 33.10 Hz [7]	510	3.59 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 2 -- Waveform details**

T3 90.0 dB nHL L 33.10 Hz [9]	986	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T5 90.0 dB nHL L 33.10 Hz [7]	Dr. Jones Protocol
T3 90.0 dB nHL L 33.10 Hz [9]	Dr. Jones Protocol

**Chart 1 -- Waveforms**

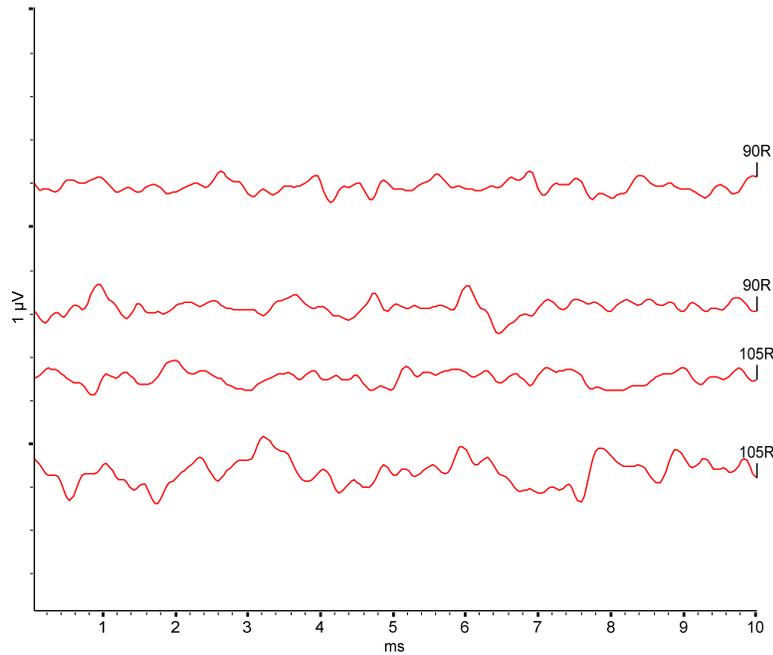

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T7 90.0 dB nHL R 33.10 Hz [1]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T8 90.0 dB nHL R 33.10 Hz [2]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T9 105.0 dB nHL R 33.10 Hz [4]	Right	105.0 dB nHL	65.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T10 105.0 dB nHL R 33.10 Hz [3]	Right	105.0 dB nHL	65.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T7 90.0 dB nHL R 33.10 Hz [1]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T8 90.0 dB nHL R 33.10 Hz [2]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T9 105.0 dB nHL R 33.10 Hz [4]	510	0.20 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T10 105.0 dB nHL R 33.10 Hz [3]	510	0.97 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Patient ID: DN29578103  
 Patient name: Buetow Branson, Pink Female  
 Date of birth: 11/28/2010  
 Gender: Female  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog


Clinic ref: MC035009306  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:26 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:30 PM**

bilateral hearing  
 no sedation

**Chart 1 -- Waveforms**

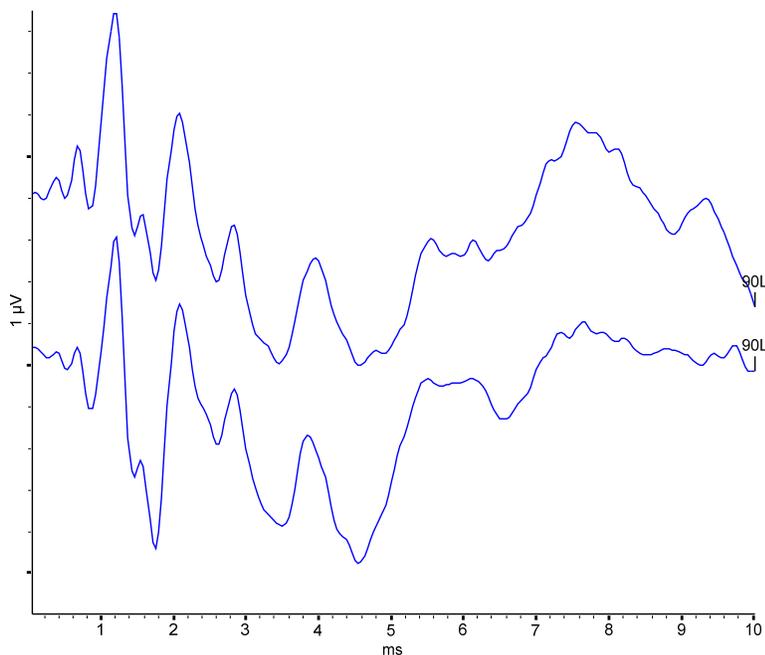

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**


Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T1 90.0 dB nHL L 33.10 Hz [2]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T2 90.0 dB nHL L 33.10 Hz [1]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T1 90.0 dB nHL L 33.10 Hz [2]	510	6.25 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T2 90.0 dB nHL L 33.10 Hz [1]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

**Chart 1 -- Waveform details**

Trace	Test set
T1 90.0 dB nHL L 33.10 Hz [2]	Dr. Jones Protocol
T2 90.0 dB nHL L 33.10 Hz [1]	Dr. Jones Protocol

**Chart 2 -- Waveforms**

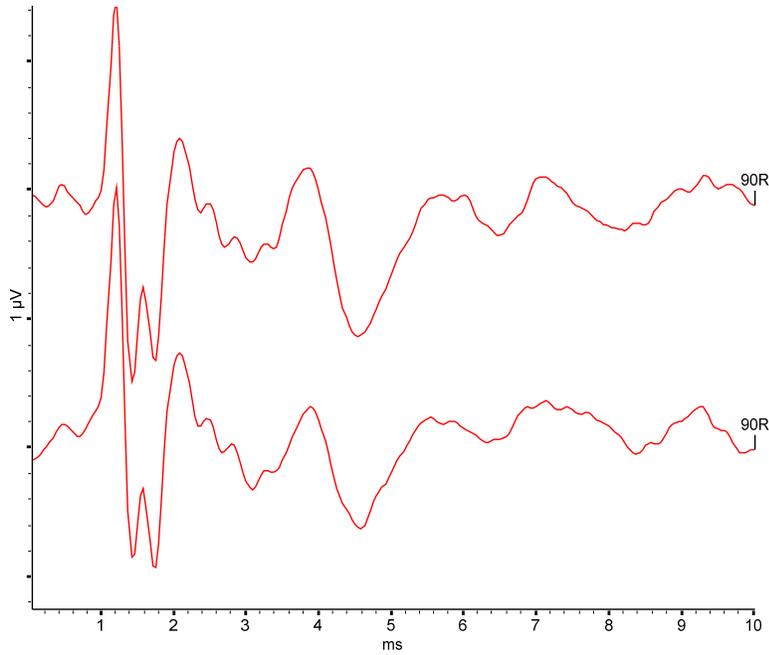

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL R 33.10 Hz [3]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T4 90.0 dB nHL R 33.10 Hz [4]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL R 33.10 Hz [3]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T4 90.0 dB nHL R 33.10 Hz [4]	510	4.67 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T3 90.0 dB nHL R 33.10 Hz [3]	Dr. Jones Protocol


Patient ID: DN29578104  
 Patient name: Buetow Branson, Red Female  
 Date of birth: 11/28/2010  
 Gender: Female  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC057529118  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:31 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:35 PM**  
 bilateral hearing  
 no sedation

**Chart 2 -- Waveforms**

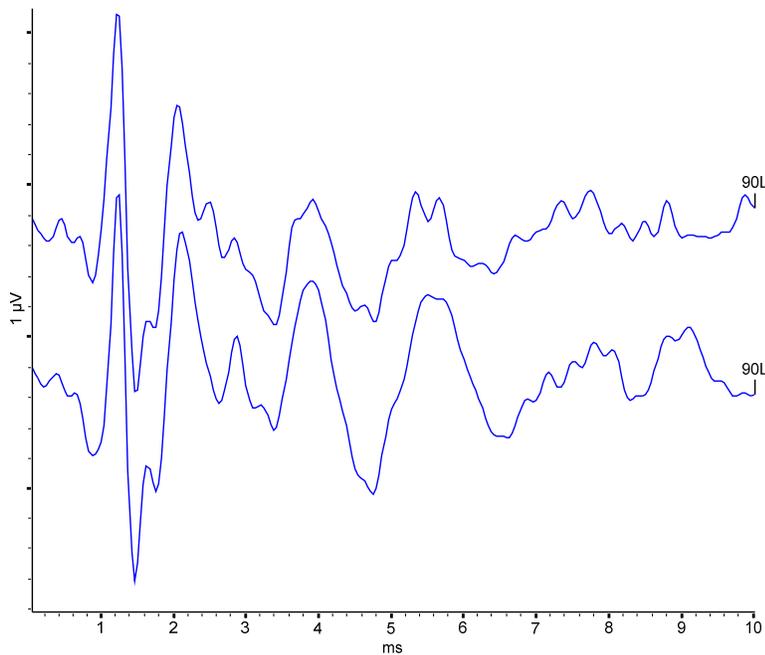

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T1 90.0 dB nHL L 33.10 Hz [4]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T2 90.0 dB nHL L 33.10 Hz [3]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T1 90.0 dB nHL L 33.10 Hz [4]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 2 -- Waveform details**

T2 90.0 dB nHL L 33.10 Hz [3]	510	3.04 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T1 90.0 dB nHL L 33.10 Hz [4]	Dr. Jones Protocol
T2 90.0 dB nHL L 33.10 Hz [3]	Dr. Jones Protocol

**Chart 1 -- Waveforms**

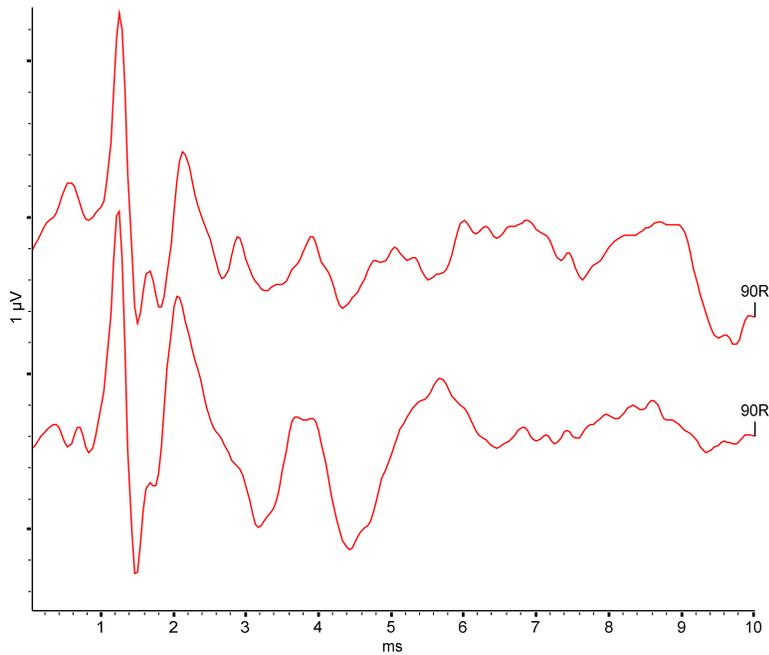

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL R 33.10 Hz [1]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T4 90.0 dB nHL R 33.10 Hz [2]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL R 33.10 Hz [1]	510	37.04 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T4 90.0 dB nHL R 33.10 Hz [2]	510	2.30 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T3 90.0 dB nHL R 33.10 Hz [1]	Dr. Jones Protocol


Patient ID: DN29578105  
 Patient name: Buetow Branson, Green Female  
 Date of birth: 11/28/2010  
 Gender: Female  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC057522033  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:38 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:41 PM**  
 bilateral hearing  
 no sedation

**Chart 1 -- Waveforms**

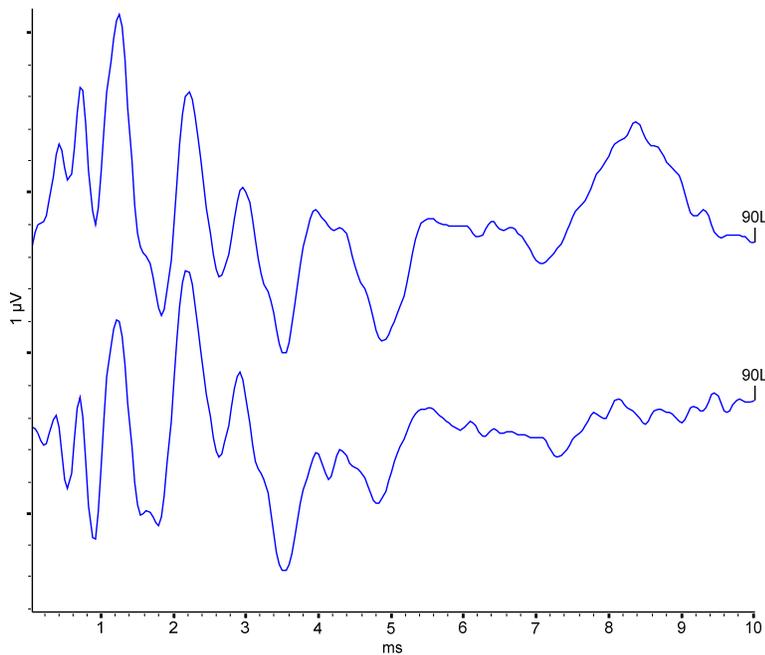

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T2 90.0 dB nHL L 33.10 Hz [1]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T1 90.0 dB nHL L 33.10 Hz [2]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T2 90.0 dB nHL L 33.10 Hz [1]	510	10.21 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 1 -- Waveform details**

T1 90.0 dB nHL L 33.10 Hz [2]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T2 90.0 dB nHL L 33.10 Hz [1]	Dr. Jones Protocol
T1 90.0 dB nHL L 33.10 Hz [2]	Dr. Jones Protocol

**Chart 2 -- Waveforms**

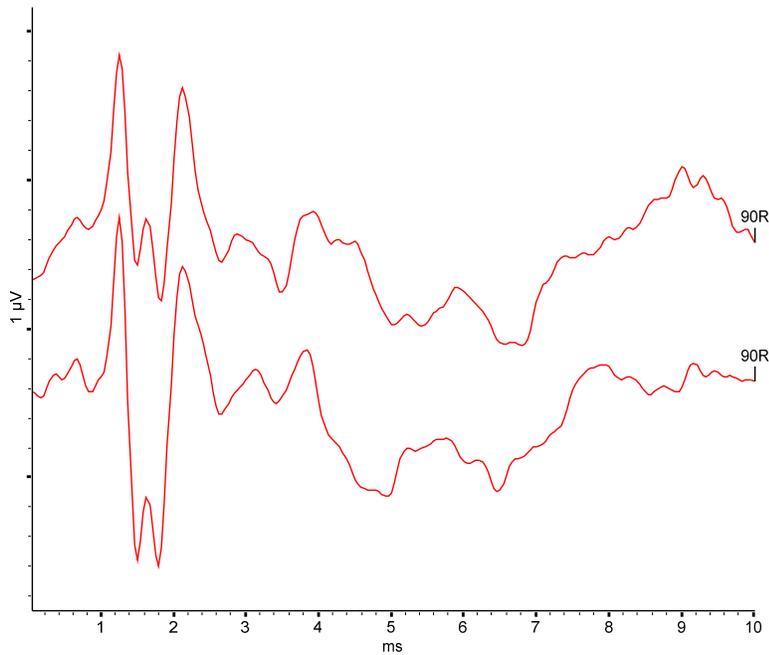

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T4 90.0 dB nHL R 33.10 Hz [3]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T3 90.0 dB nHL R 33.10 Hz [4]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T4 90.0 dB nHL R 33.10 Hz [3]	510	2.11 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T3 90.0 dB nHL R 33.10 Hz [4]	510	0.20 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T4 90.0 dB nHL R 33.10 Hz [3]	Dr. Jones Protocol


Patient ID: DN29578106  
 Patient name: Buetow Branson, Orange Male  
 Date of birth: 11/28/2010  
 Gender: Male  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC057380055  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:44 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:58 PM**  
 bilateral hearing  
 no sedation

**Chart 2 -- Waveforms**

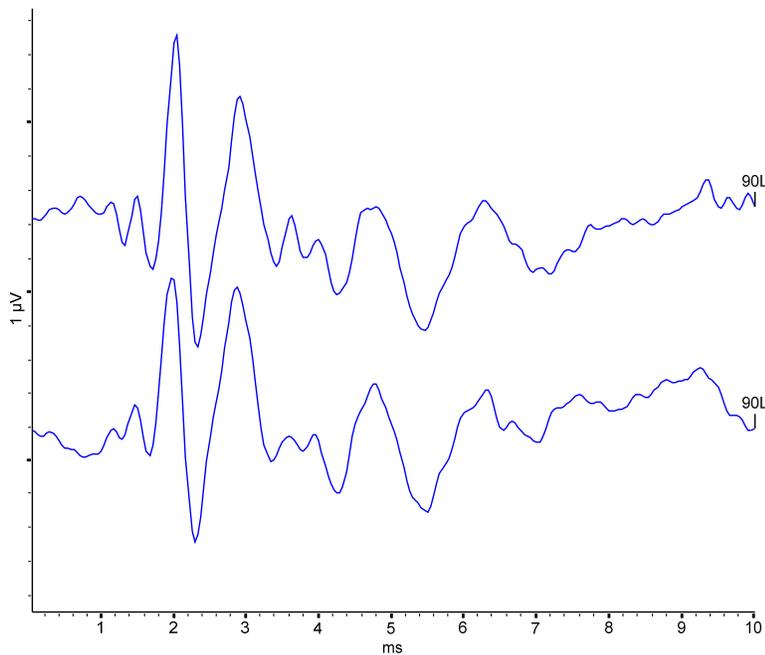

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**


Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T14 90.0 dB nHL L 33.10 Hz [15]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T15 90.0 dB nHL L 33.10 Hz [14]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T14 90.0 dB nHL L 33.10 Hz [15]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T15 90.0 dB nHL L 33.10 Hz [14]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

**Chart 2 -- Waveform details**

Trace	Test set
T14 90.0 dB nHL L 33.10 Hz [15]	Dr. Jones Protocol
T15 90.0 dB nHL L 33.10 Hz [14]	Dr. Jones Protocol

**Chart 1 -- Waveforms**

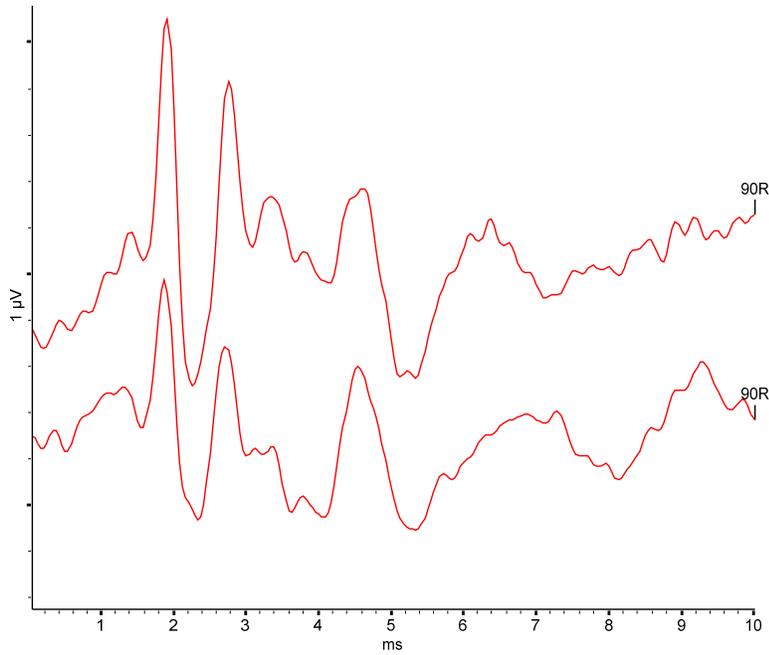

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T12 90.0 dB nHL R 33.10 Hz [9]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T7 90.0 dB nHL R 33.10 Hz [10]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T12 90.0 dB nHL R 33.10 Hz [9]	510	0.39 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T7 90.0 dB nHL R 33.10 Hz [10]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T12 90.0 dB nHL R 33.10 Hz [9]	Dr. Jones Protocol
T7 90.0 dB nHL R 33.10 Hz [10]	Dr. Jones Protocol


Patient ID: DN29578107  
 Patient name: Buetow Branson, Black Male  
 Date of birth: 11/28/2010  
 Gender: Male  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC057531603  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 3:02 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 3:08 PM**  
 bilateral hearing  
 no sedation

**Chart 1 -- Waveforms**

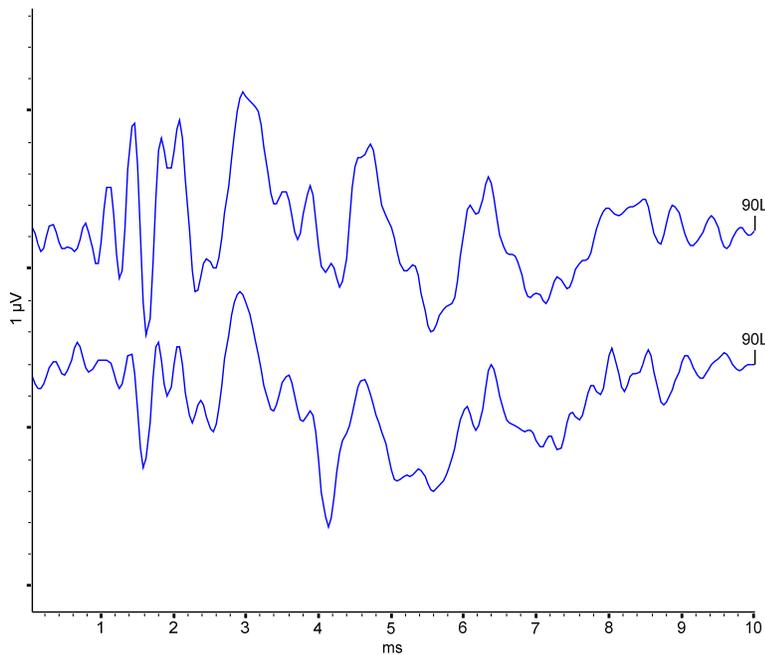

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**


Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL L 33.10 Hz [4]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T2 90.0 dB nHL L 33.10 Hz [2]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL L 33.10 Hz [4]	510	0.39 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T2 90.0 dB nHL L 33.10 Hz [2]	680	4.90 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

**Chart 1 -- Waveform details**

Trace	Test set
T3 90.0 dB nHL L 33.10 Hz [4]	Dr. Jones Protocol
T2 90.0 dB nHL L 33.10 Hz [2]	Dr. Jones Protocol

**Chart 2 -- Waveforms**

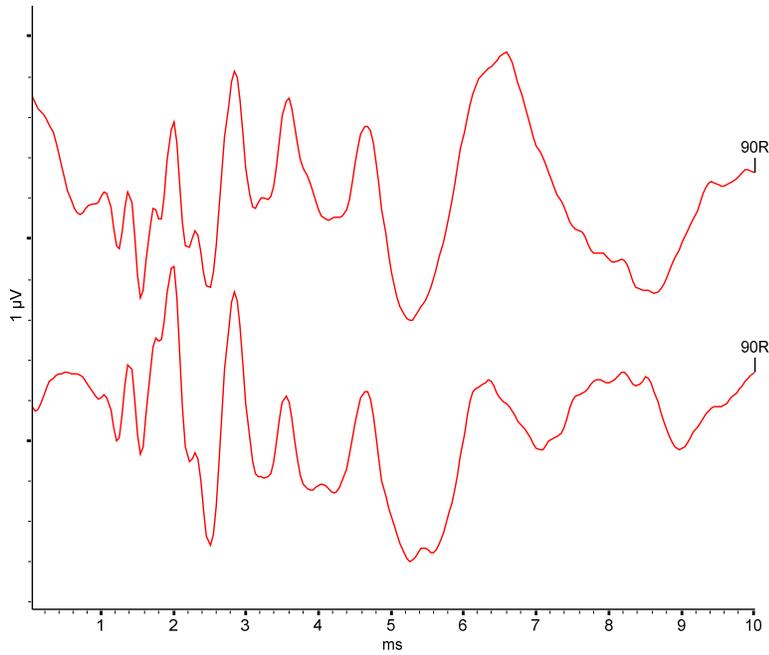

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T5 90.0 dB nHL R 33.10 Hz [5]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T6 90.0 dB nHL R 33.10 Hz [6]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T5 90.0 dB nHL R 33.10 Hz [5]	510	1.92 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T6 90.0 dB nHL R 33.10 Hz [6]	510	0.20 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T5 90.0 dB nHL R 33.10 Hz [5]	Dr. Jones Protocol
T6 90.0 dB nHL R 33.10 Hz [6]	Dr. Jones Protocol