

Patient ID: DN29578102
Patient name: Buetow Branson, Blue Male
Date of birth: 11/28/2010
Gender: Male
Gestational age: n/a
Keywords: Australian Cattle Dog

Clinic ref: MC035026809
Site: Canine Companions Veterinary Hospital
Examiner: Joanna Jones, DVM
Exam date: 1/12/2011 2:16 PM
Age on exam date: 1 month

Patient Notes

AEP, 1/12/2011 2:23 PM

Unilateral deaf - right ear
no sedation.

Chart 2 -- Waveforms

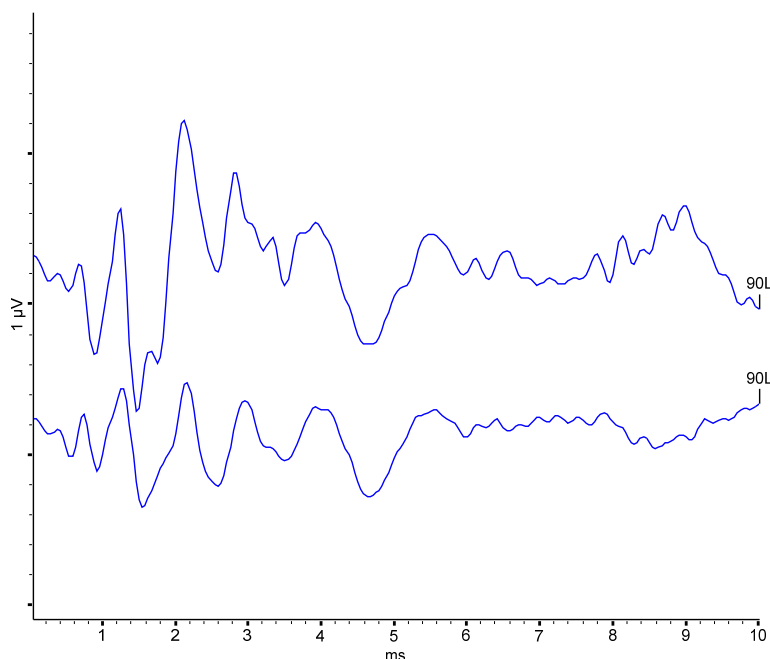


Chart 2 -- Measurements

This measurement table has not been printed because it is blank.

Chart 2 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T5 90.0 dB nHL L 33.10 Hz [7]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T3 90.0 dB nHL L 33.10 Hz [9]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T5 90.0 dB nHL L 33.10 Hz [7]	510	3.59 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

Chart 2 -- Waveform details

T3 90.0 dB nHL L 33.10 Hz [9]	986	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T5 90.0 dB nHL L 33.10 Hz [7]	Dr. Jones Protocol
T3 90.0 dB nHL L 33.10 Hz [9]	Dr. Jones Protocol

Chart 1 -- Waveforms

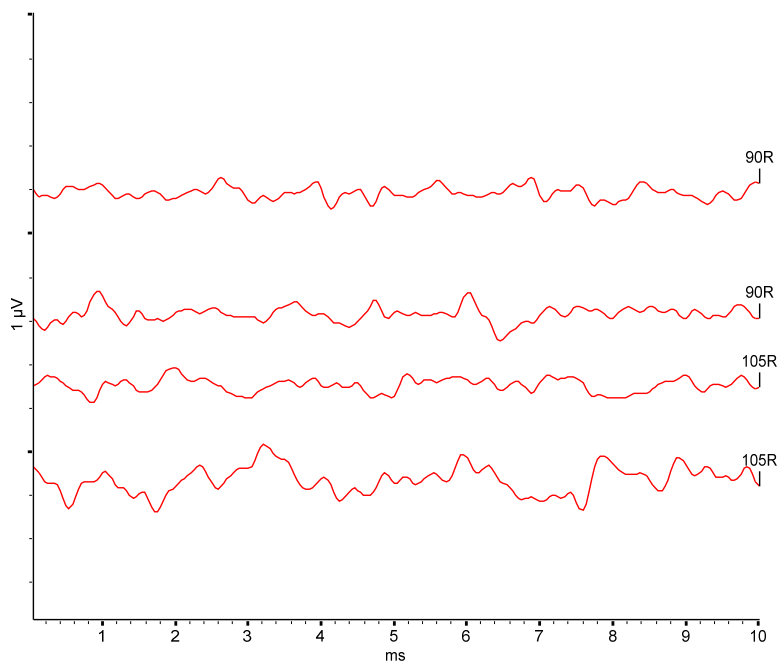


Chart 1 -- Measurements

This measurement table has not been printed because it is blank.

Chart 1 -- Waveform details

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T7 90.0 dB nHL R 33.10 Hz [1]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T8 90.0 dB nHL R 33.10 Hz [2]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T9 105.0 dB nHL R 33.10 Hz [4]	Right	105.0 dB nHL	65.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T10 105.0 dB nHL R 33.10 Hz [3]	Right	105.0 dB nHL	65.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T7 90.0 dB nHL R 33.10 Hz [1]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T8 90.0 dB nHL R 33.10 Hz [2]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T9 105.0 dB nHL R 33.10 Hz [4]	510	0.20 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T10 105.0 dB nHL R 33.10 Hz [3]	510	0.97 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Chart 1 -- Waveform details

Trace	Test set
T7 90.0 dB nHL R 33.10 Hz [1]	Dr. Jones Protocol
T8 90.0 dB nHL R 33.10 Hz [2]	Dr. Jones Protocol
T9 105.0 dB nHL R 33.10 Hz [4]	Dr. Jones Protocol
T10 105.0 dB nHL R 33.10 Hz [3]	Dr. Jones Protocol