


Patient ID: DN29578104  
 Patient name: Buetow Branson, Red Female  
 Date of birth: 11/28/2010  
 Gender: Female  
 Gestational age: n/a  
 Keywords: Australian Cattle Dog

Clinic ref: MC057529118  
 Site: Canine Companions Veterinary Hospital  
 Examiner: Joanna Jones, DVM  
 Exam date: 1/12/2011 2:31 PM  
 Age on exam date: 1 month

**Patient Notes**

**AEP, 1/12/2011 2:35 PM**  
 bilateral hearing  
 no sedation

**Chart 2 -- Waveforms**

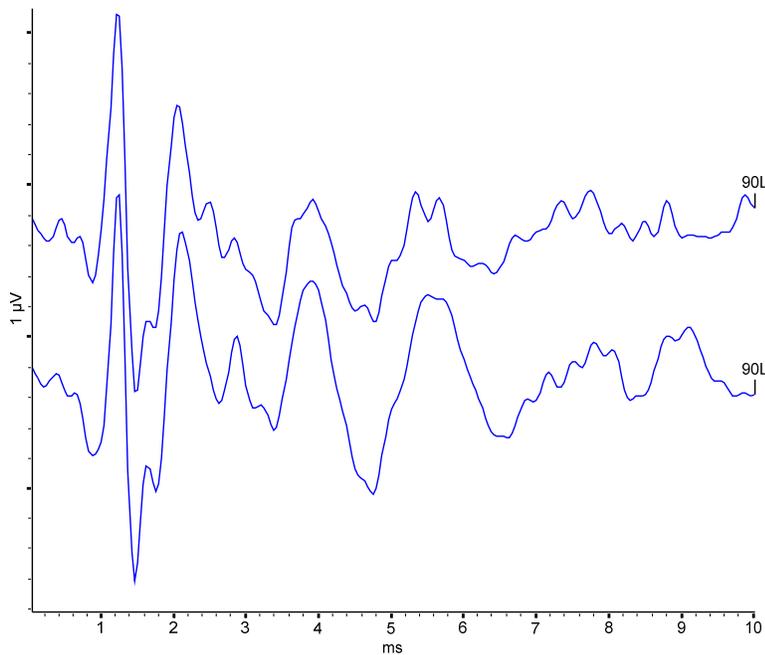

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T1 90.0 dB nHL L 33.10 Hz [4]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T2 90.0 dB nHL L 33.10 Hz [3]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T1 90.0 dB nHL L 33.10 Hz [4]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 2 -- Waveform details**

T2 90.0 dB nHL L 33.10 Hz [3]	510	3.04 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T1 90.0 dB nHL L 33.10 Hz [4]	Dr. Jones Protocol
T2 90.0 dB nHL L 33.10 Hz [3]	Dr. Jones Protocol

**Chart 1 -- Waveforms**

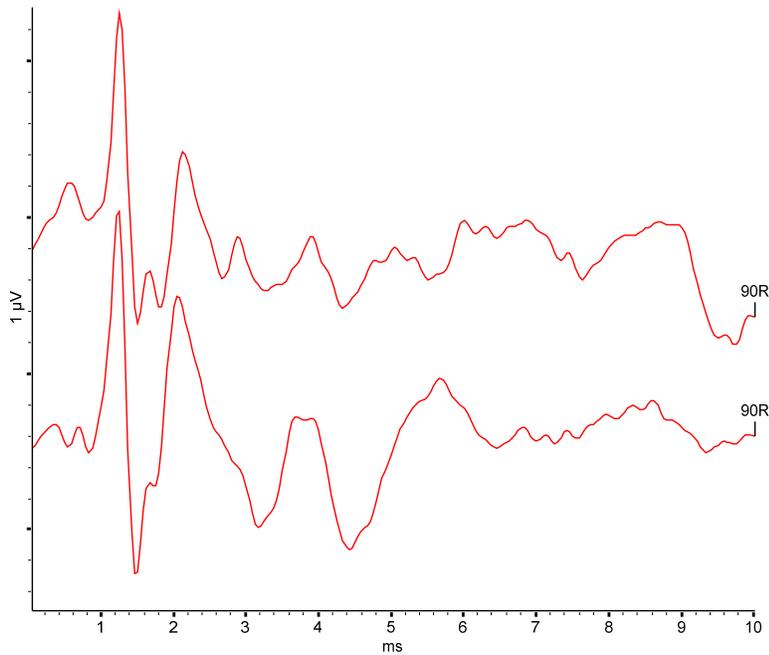

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T3 90.0 dB nHL R 33.10 Hz [1]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T4 90.0 dB nHL R 33.10 Hz [2]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T3 90.0 dB nHL R 33.10 Hz [1]	510	37.04 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T4 90.0 dB nHL R 33.10 Hz [2]	510	2.30 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T3 90.0 dB nHL R 33.10 Hz [1]	Dr. Jones Protocol

**Chart 1 -- Waveform details**

T4 90.0 dB nHL R 33.10 Hz [2]	Dr. Jones Protocol
-------------------------------	--------------------